How to use i-scope analyzer

Please read and follow this instruction carefully

1)The method of connection to i-scope and computer

Connect the cable to stethoscope's output terminal and PC Line n OR Audio in terminal.

.

※ Please use 3m length cable when connect with PC.

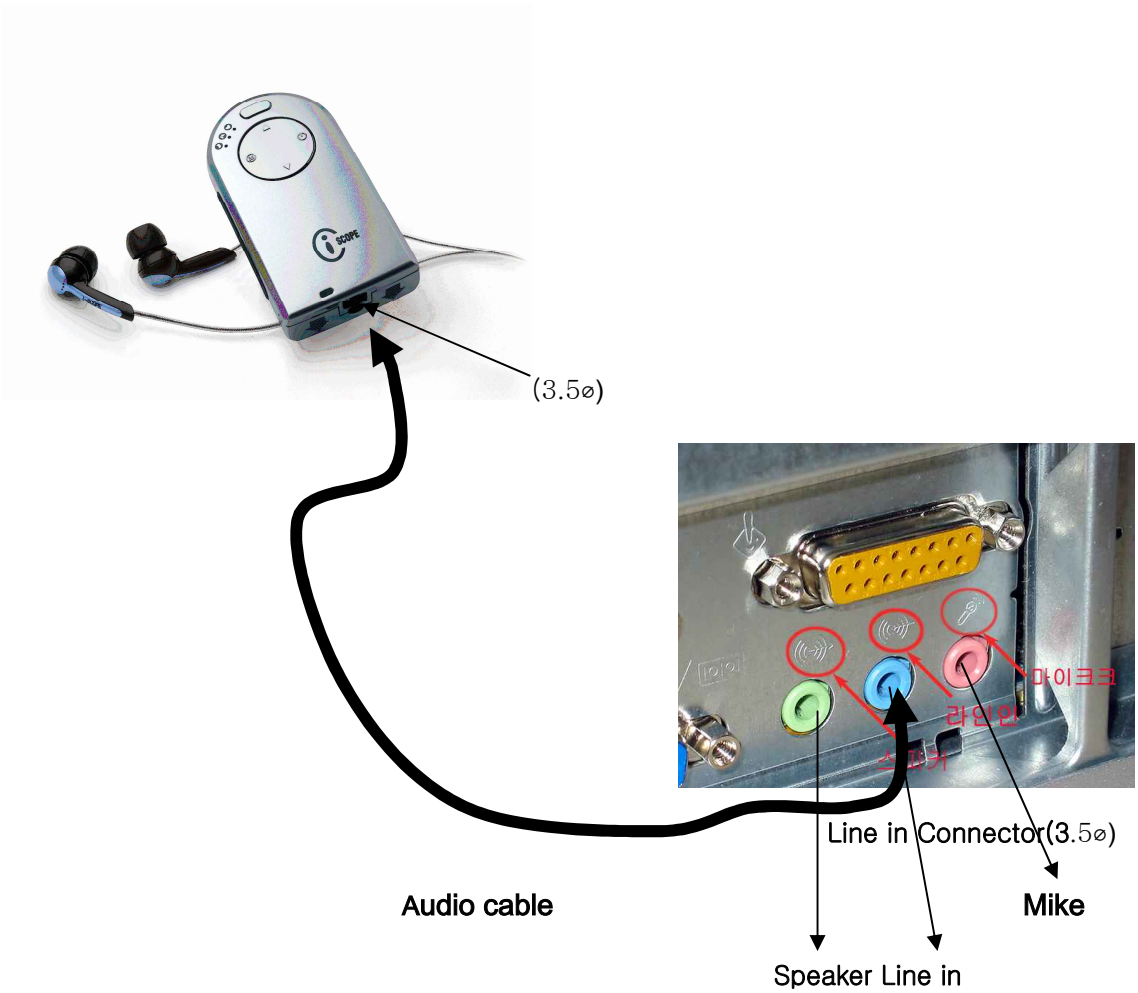

Icon on the computer

- Speaker – Headphone icon
- Mike- Mike icon
- Line In – Half circle

Turn on computer

1) After connect like above, turn on a computer and start Windows

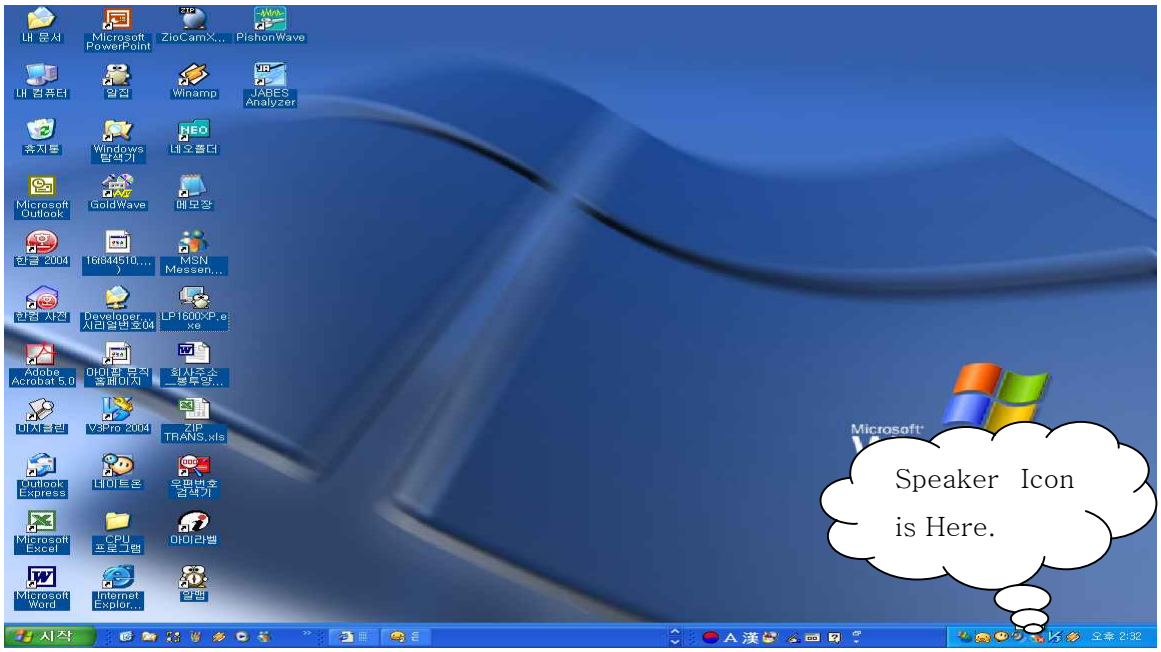

2) Double click a speaker icon on the right bottom(if muted, delete it)

3) Master volume or master control panel is appeared.

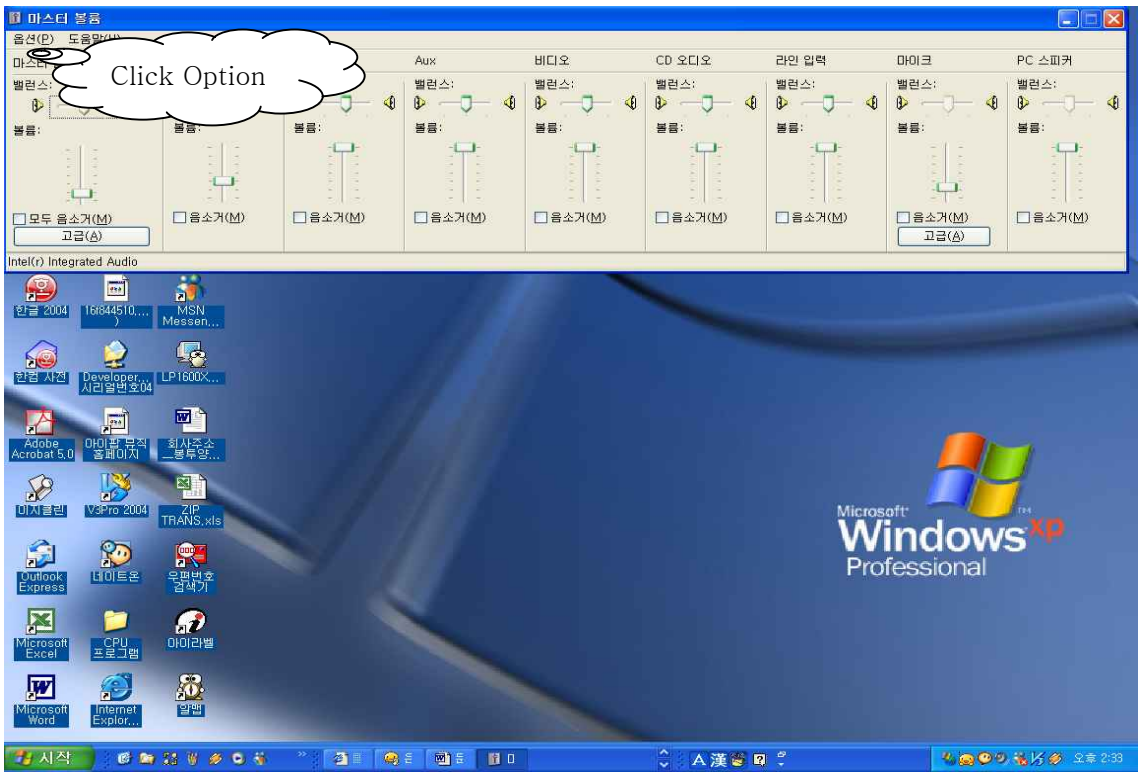

4) Click Option

5) Choose Properties.

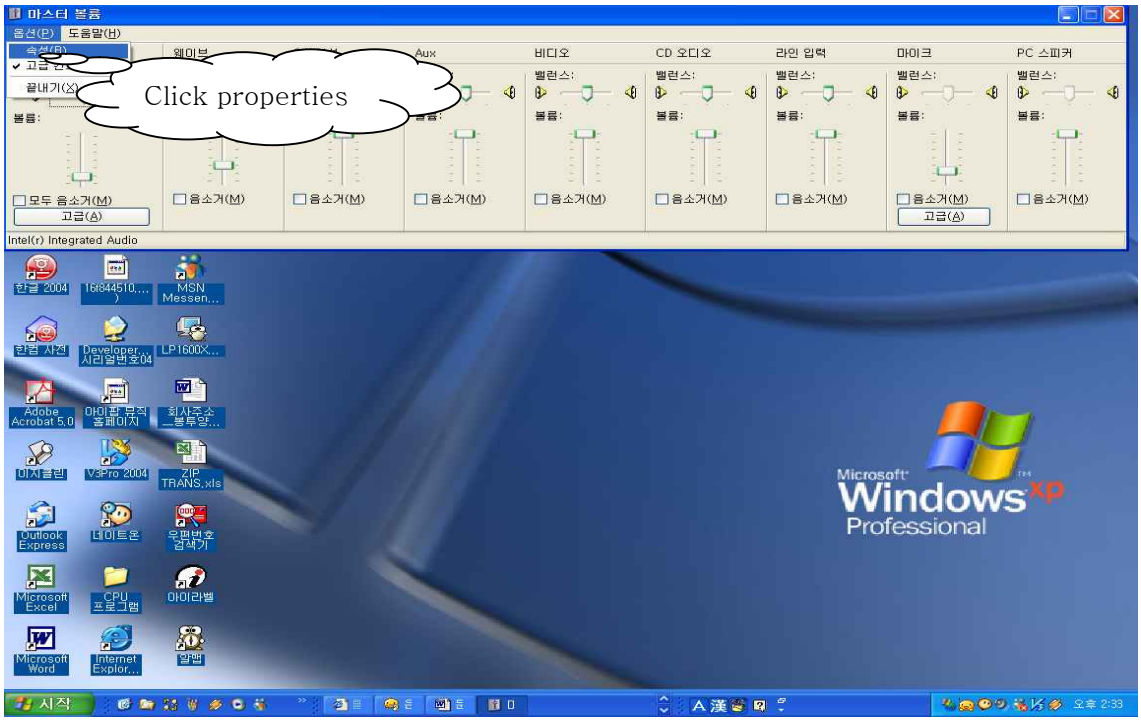

6) After choose properties, you can see a pop up window include Mixer, volume control and play&record option

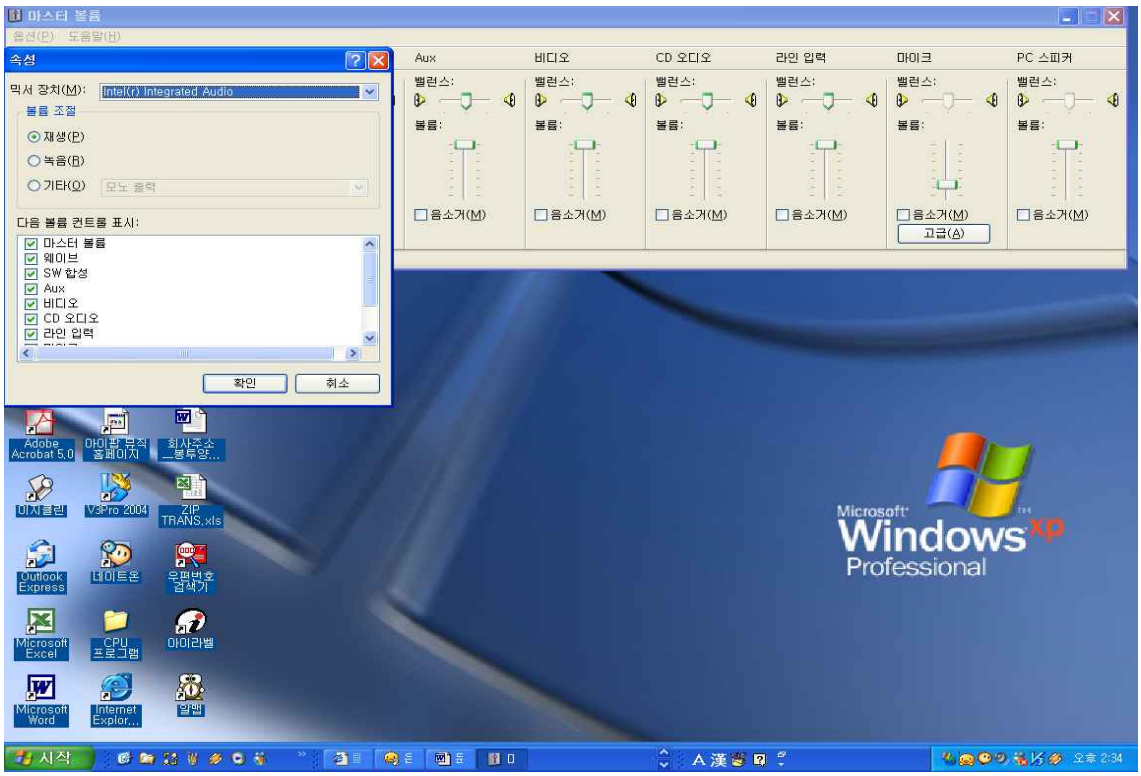

7) Click Record

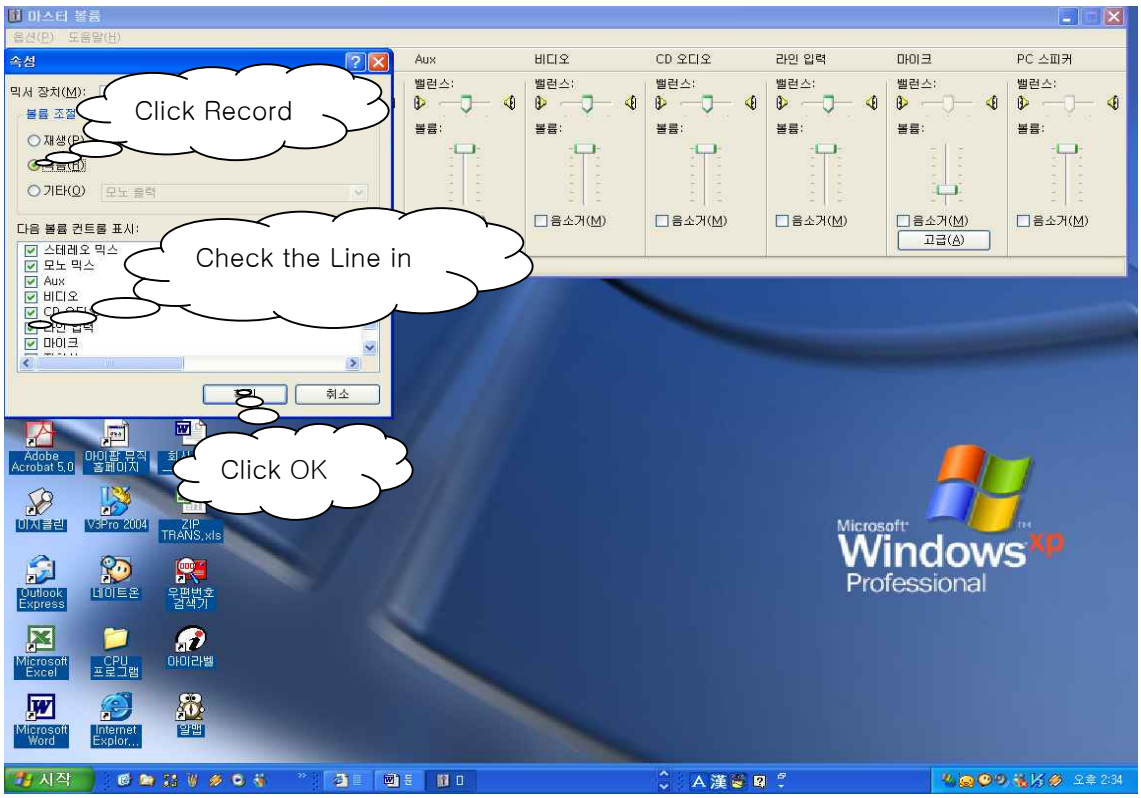

8) Please check Line In or Mike(If line in is not there) and Click OK button

9) Volume control panel is appeared

10) Please control volume for your intention

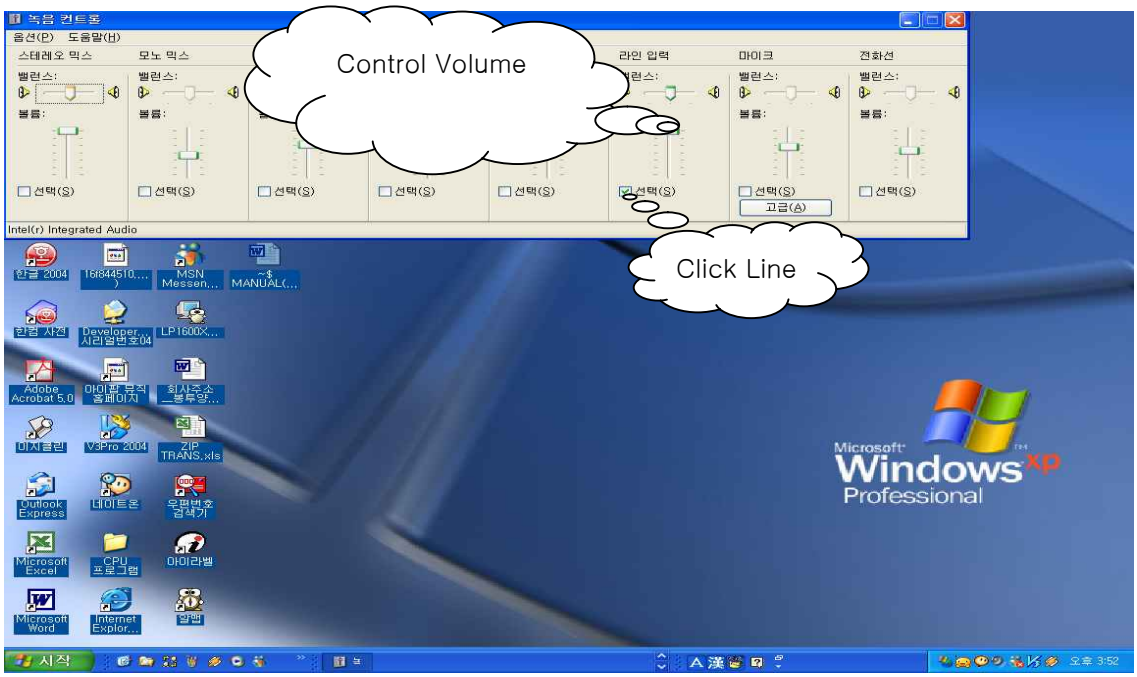

11) Please click Line in Or mike

12) After check the Line in or Mike, click option button on left upper side

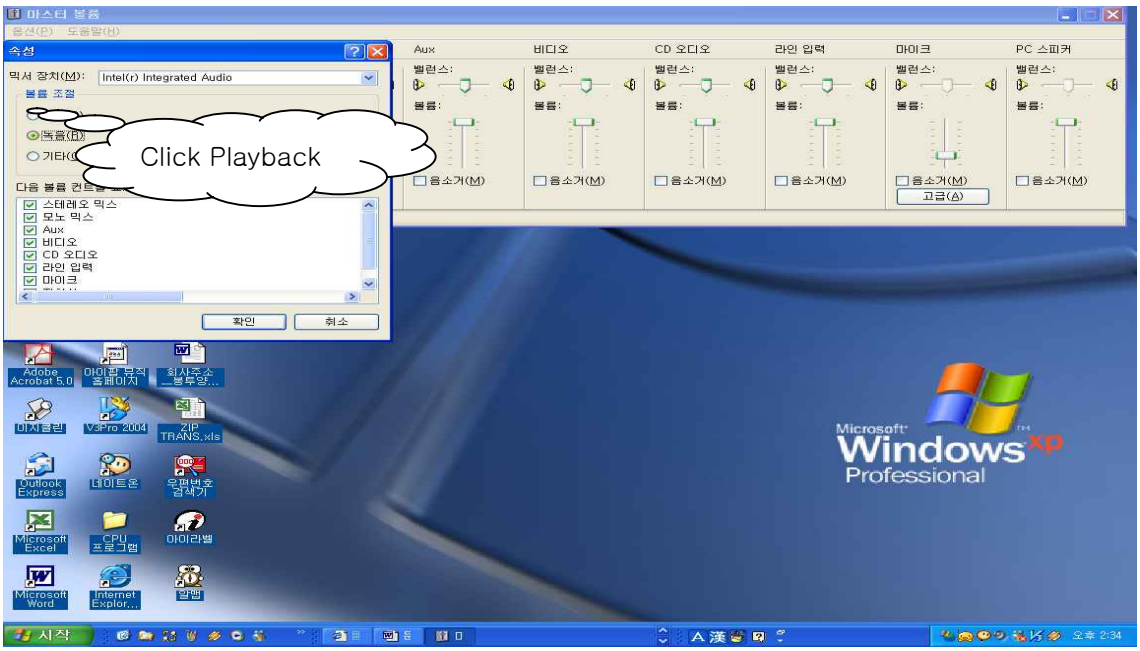

13) Click Playback

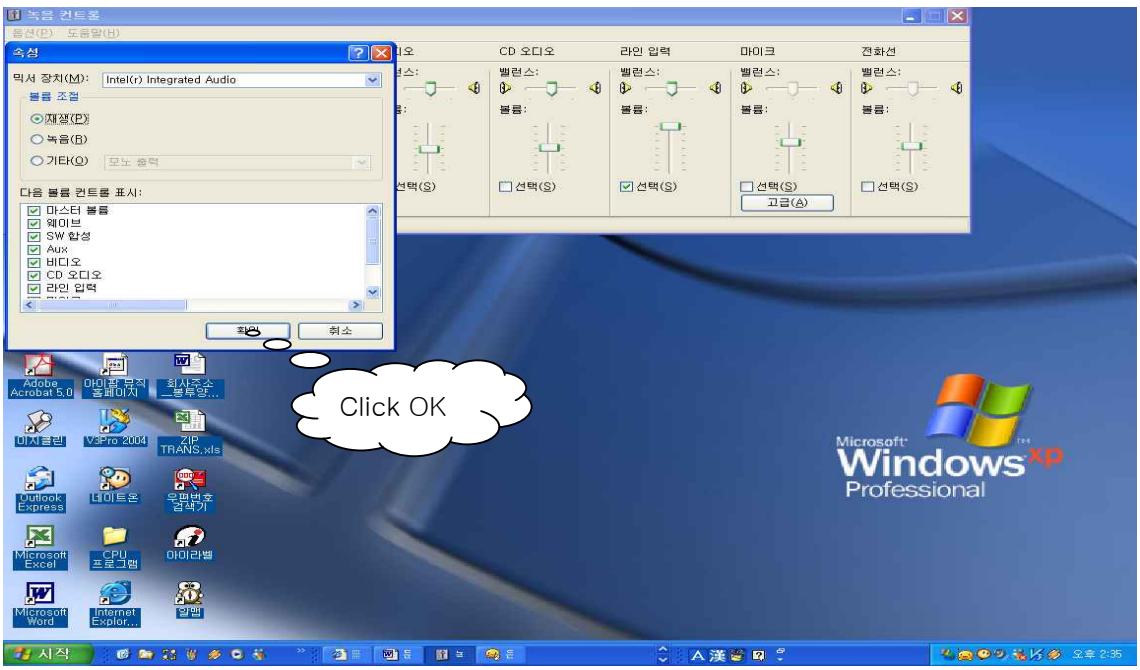

13) Please check Master Volume, Mic and Line in and OK button

14) Check the mute button is checked, if mute is selected, please remove it.

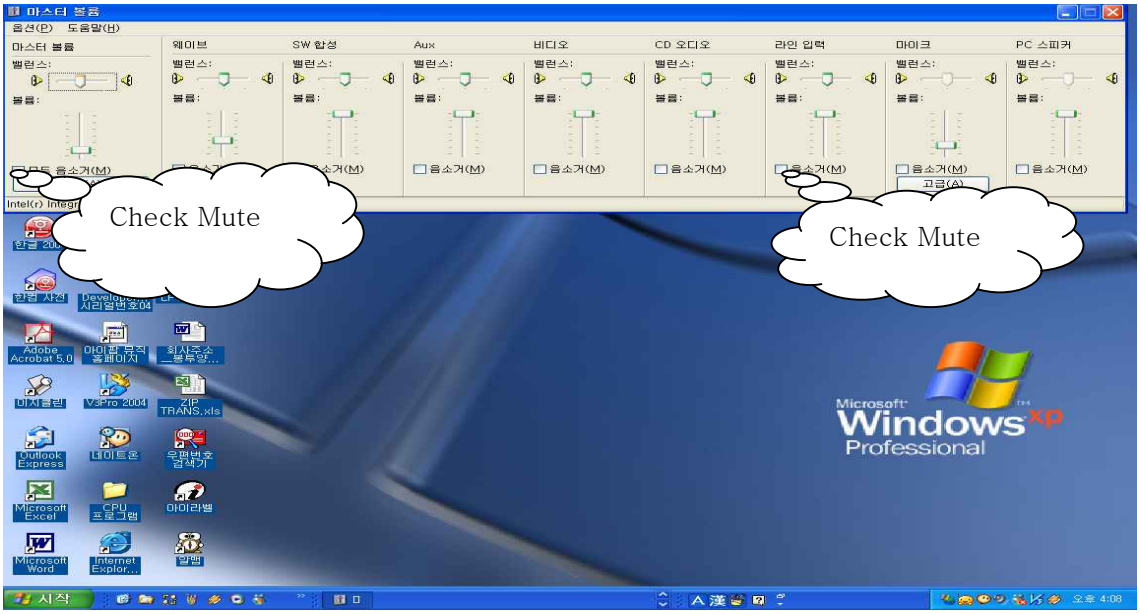

17) After finish everything, please start iscope analyzer.
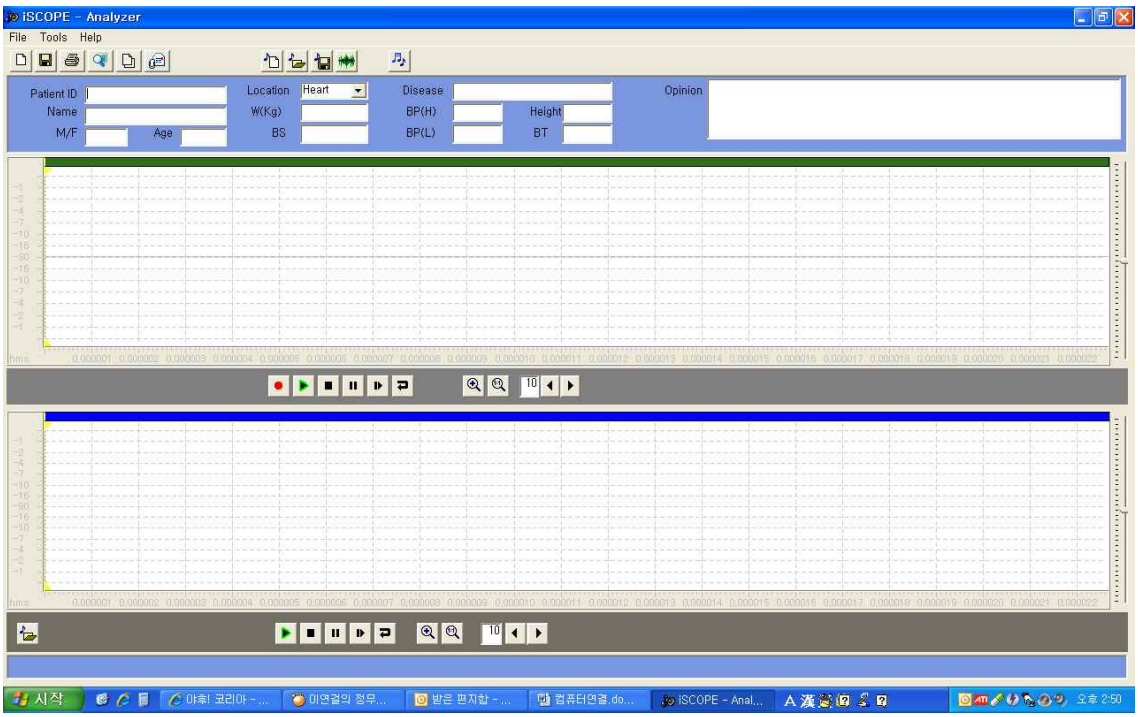
19) You can see below program on your monitor.